

2010-11-16

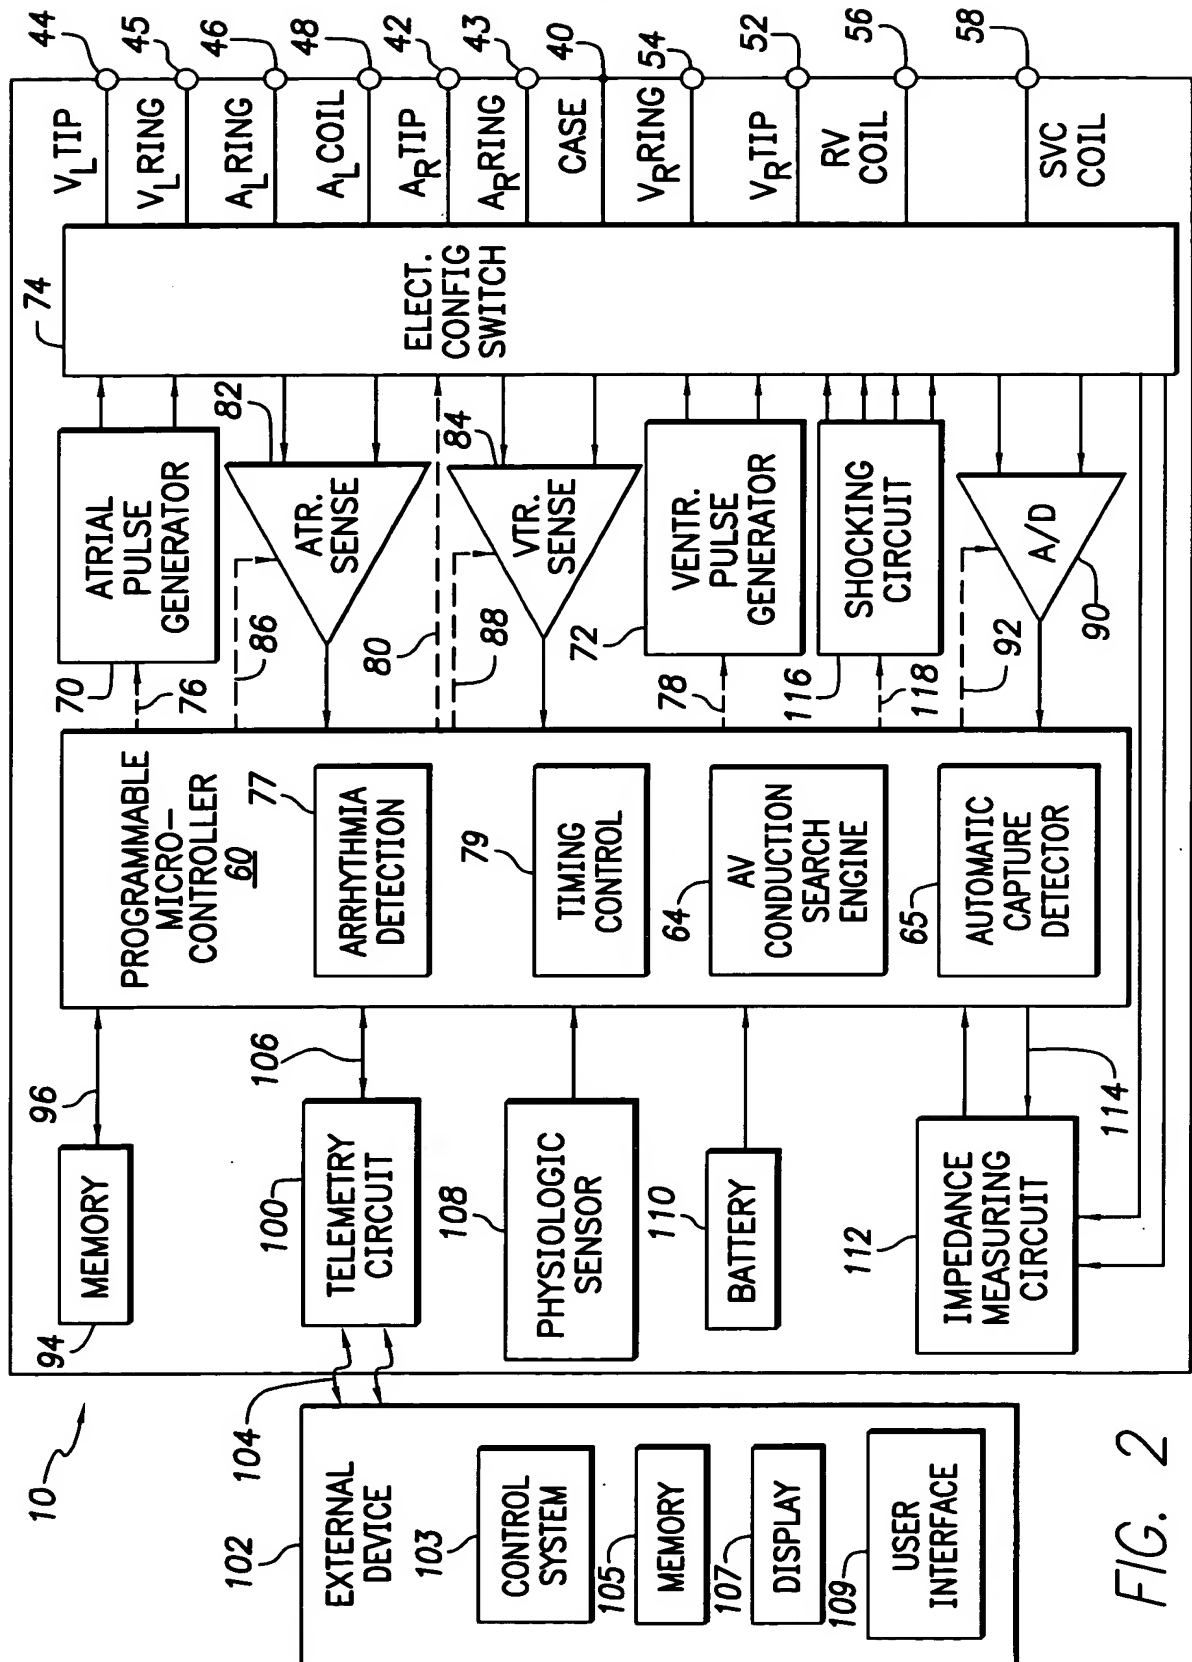
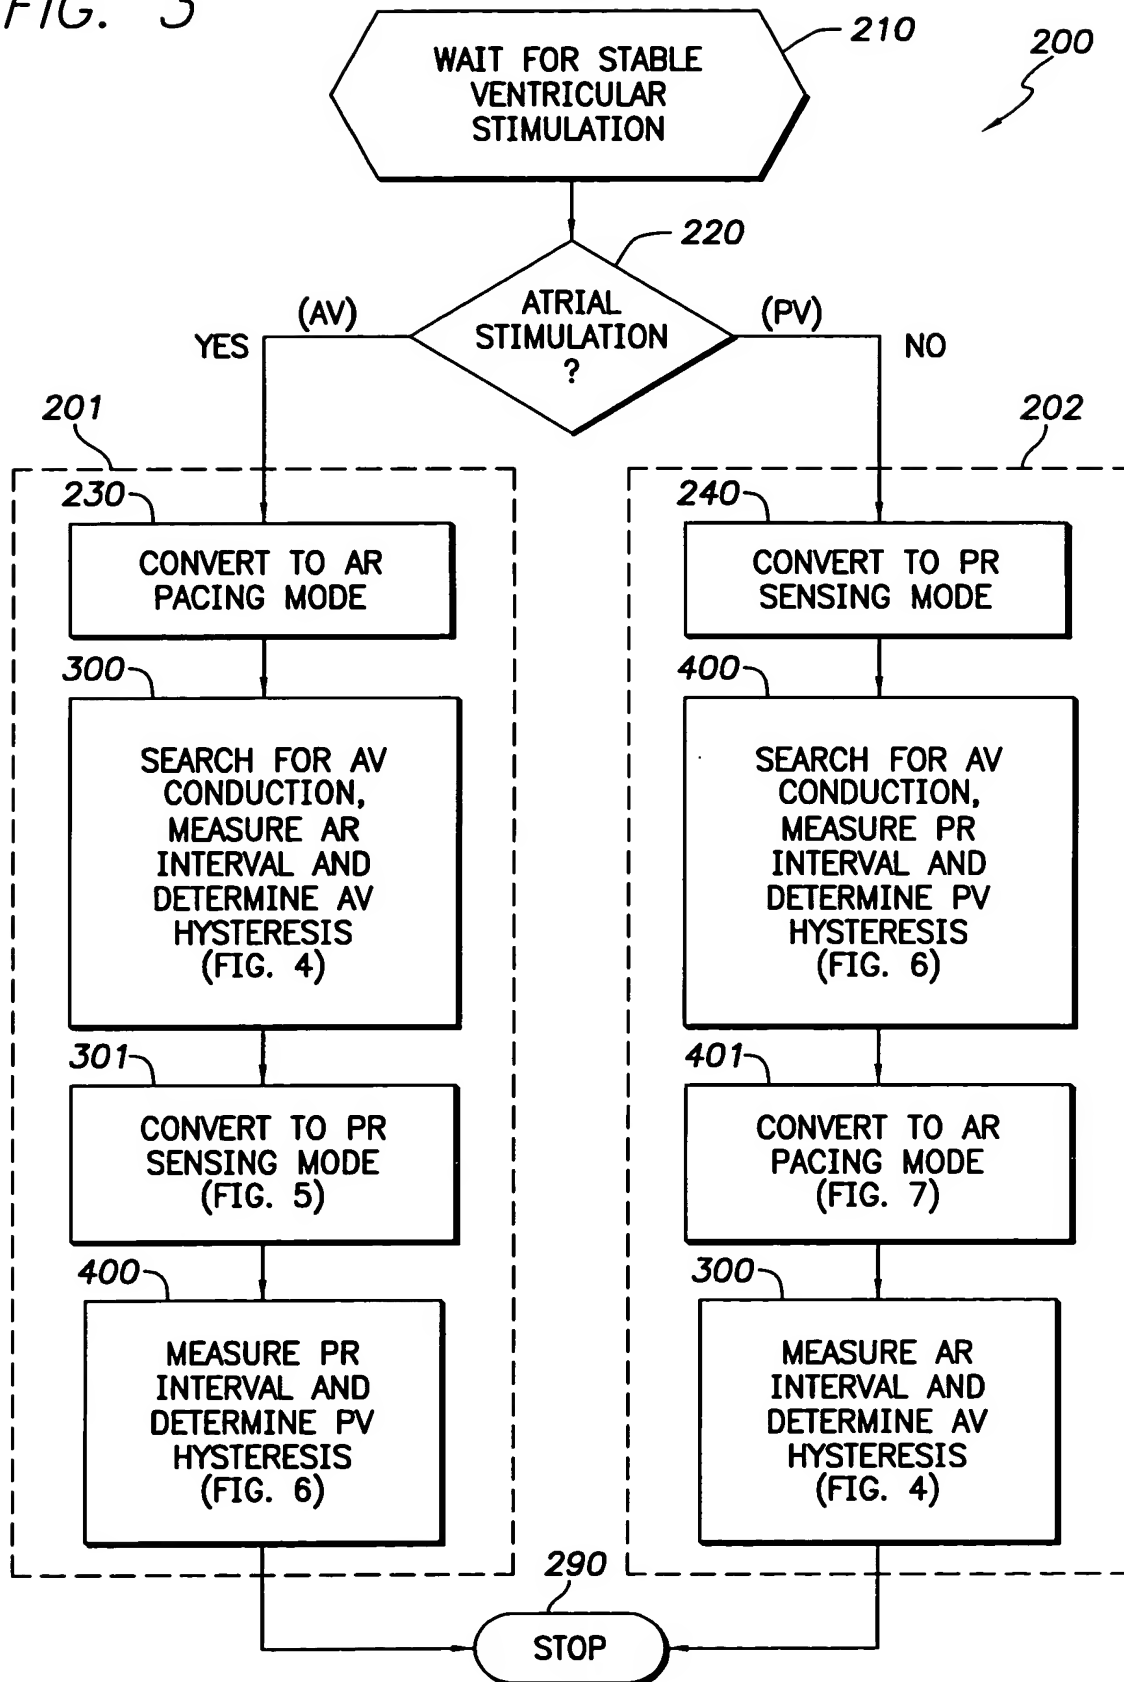


FIG. 3

3/9



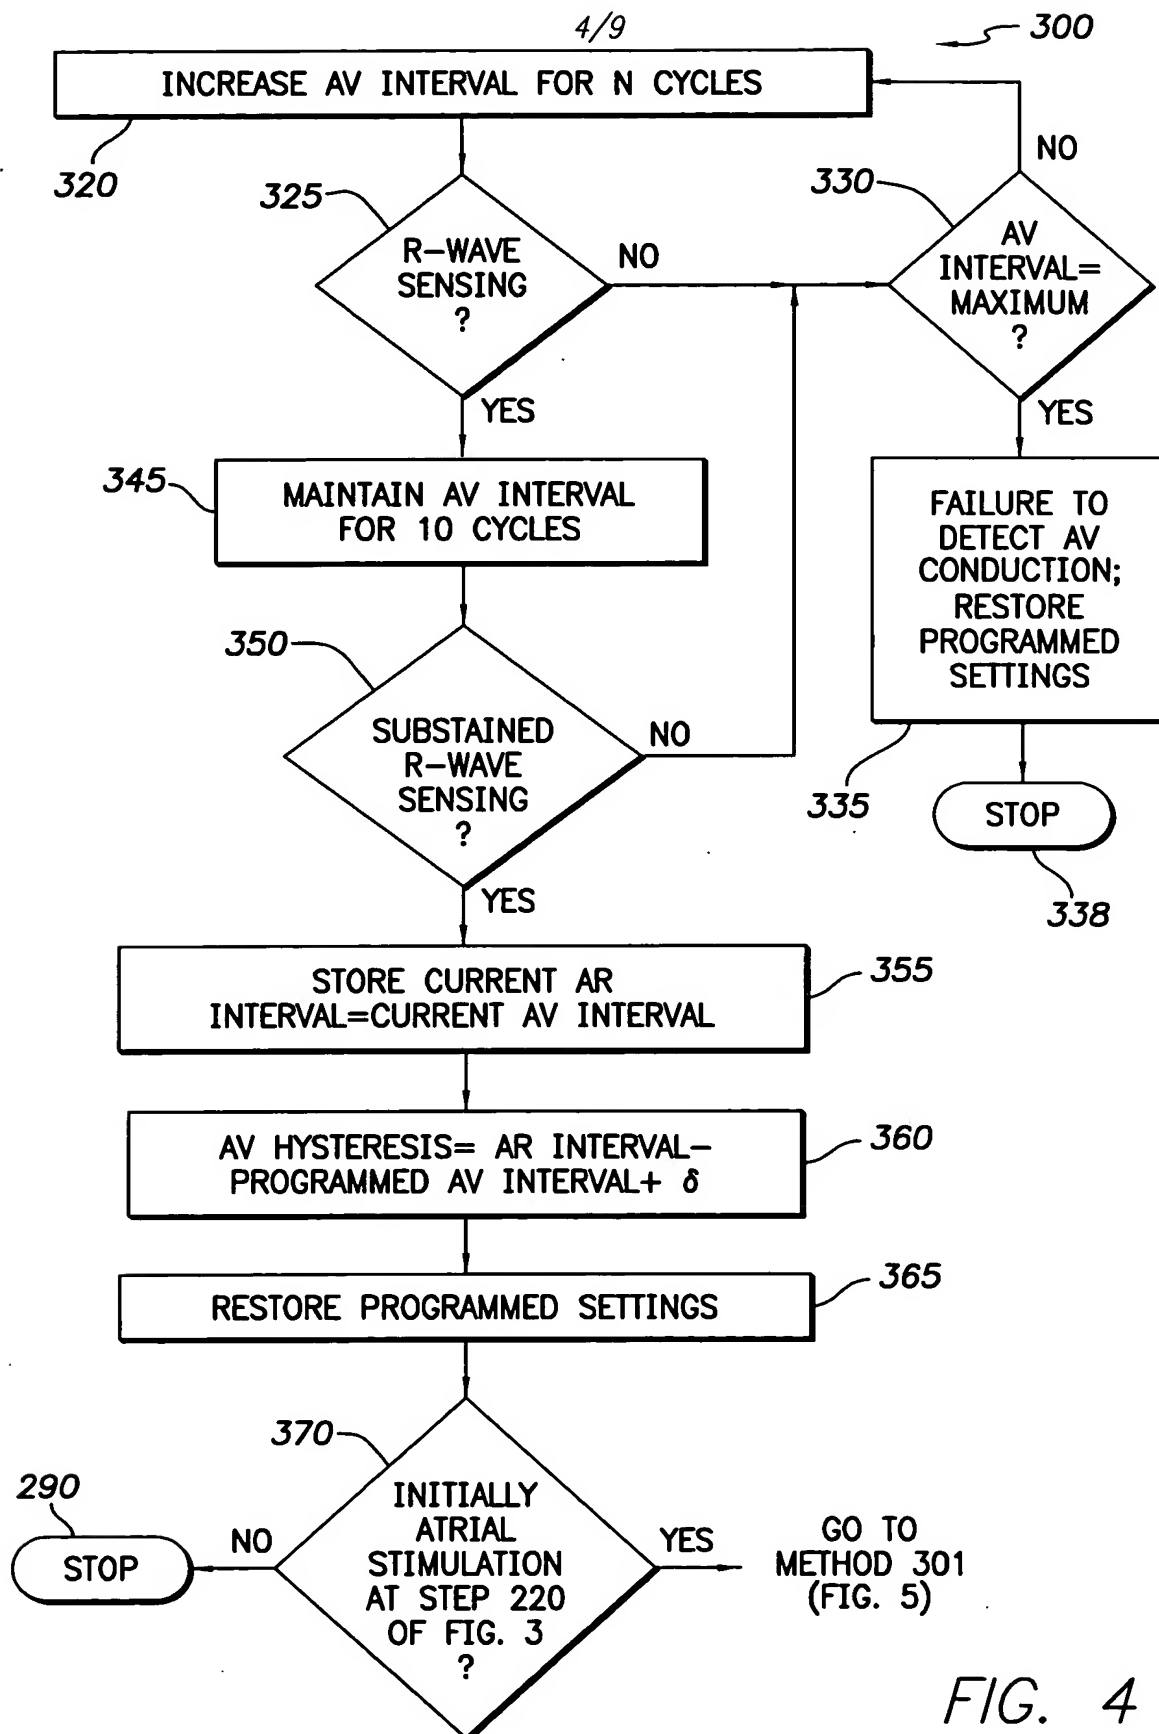
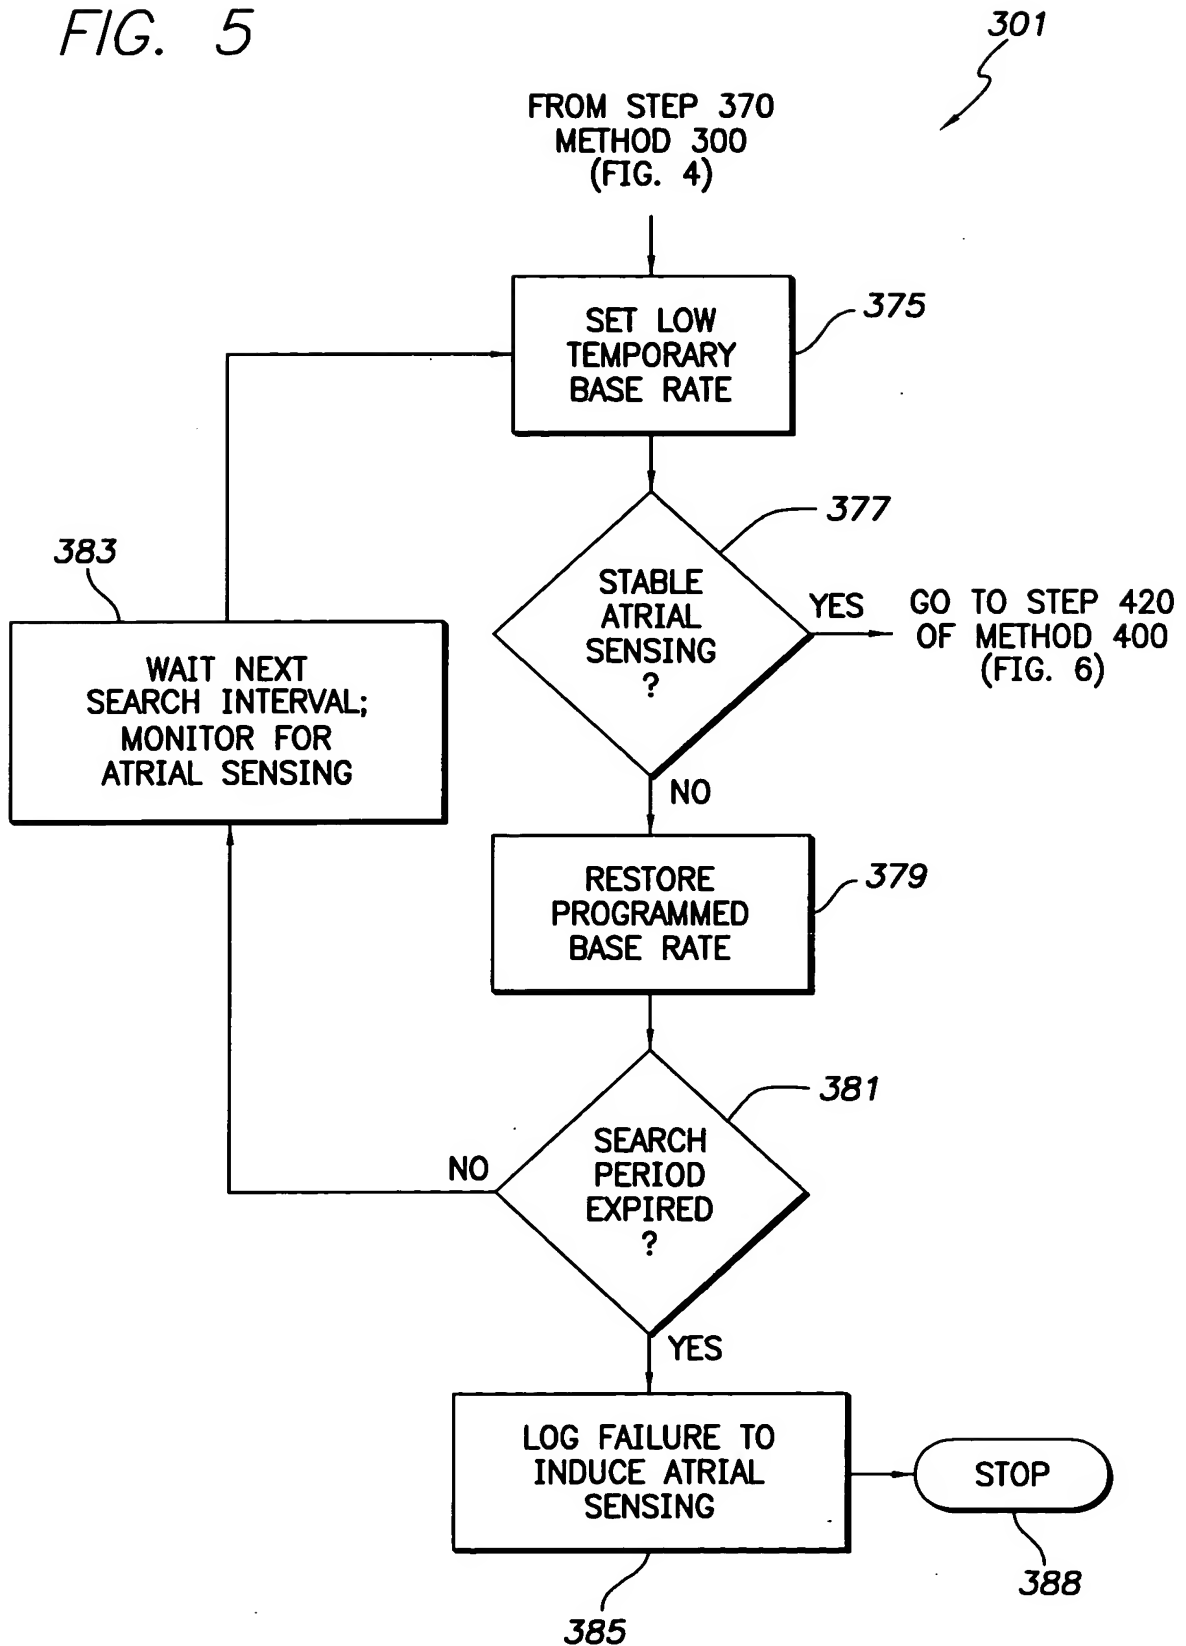


FIG. 4

FIG. 5



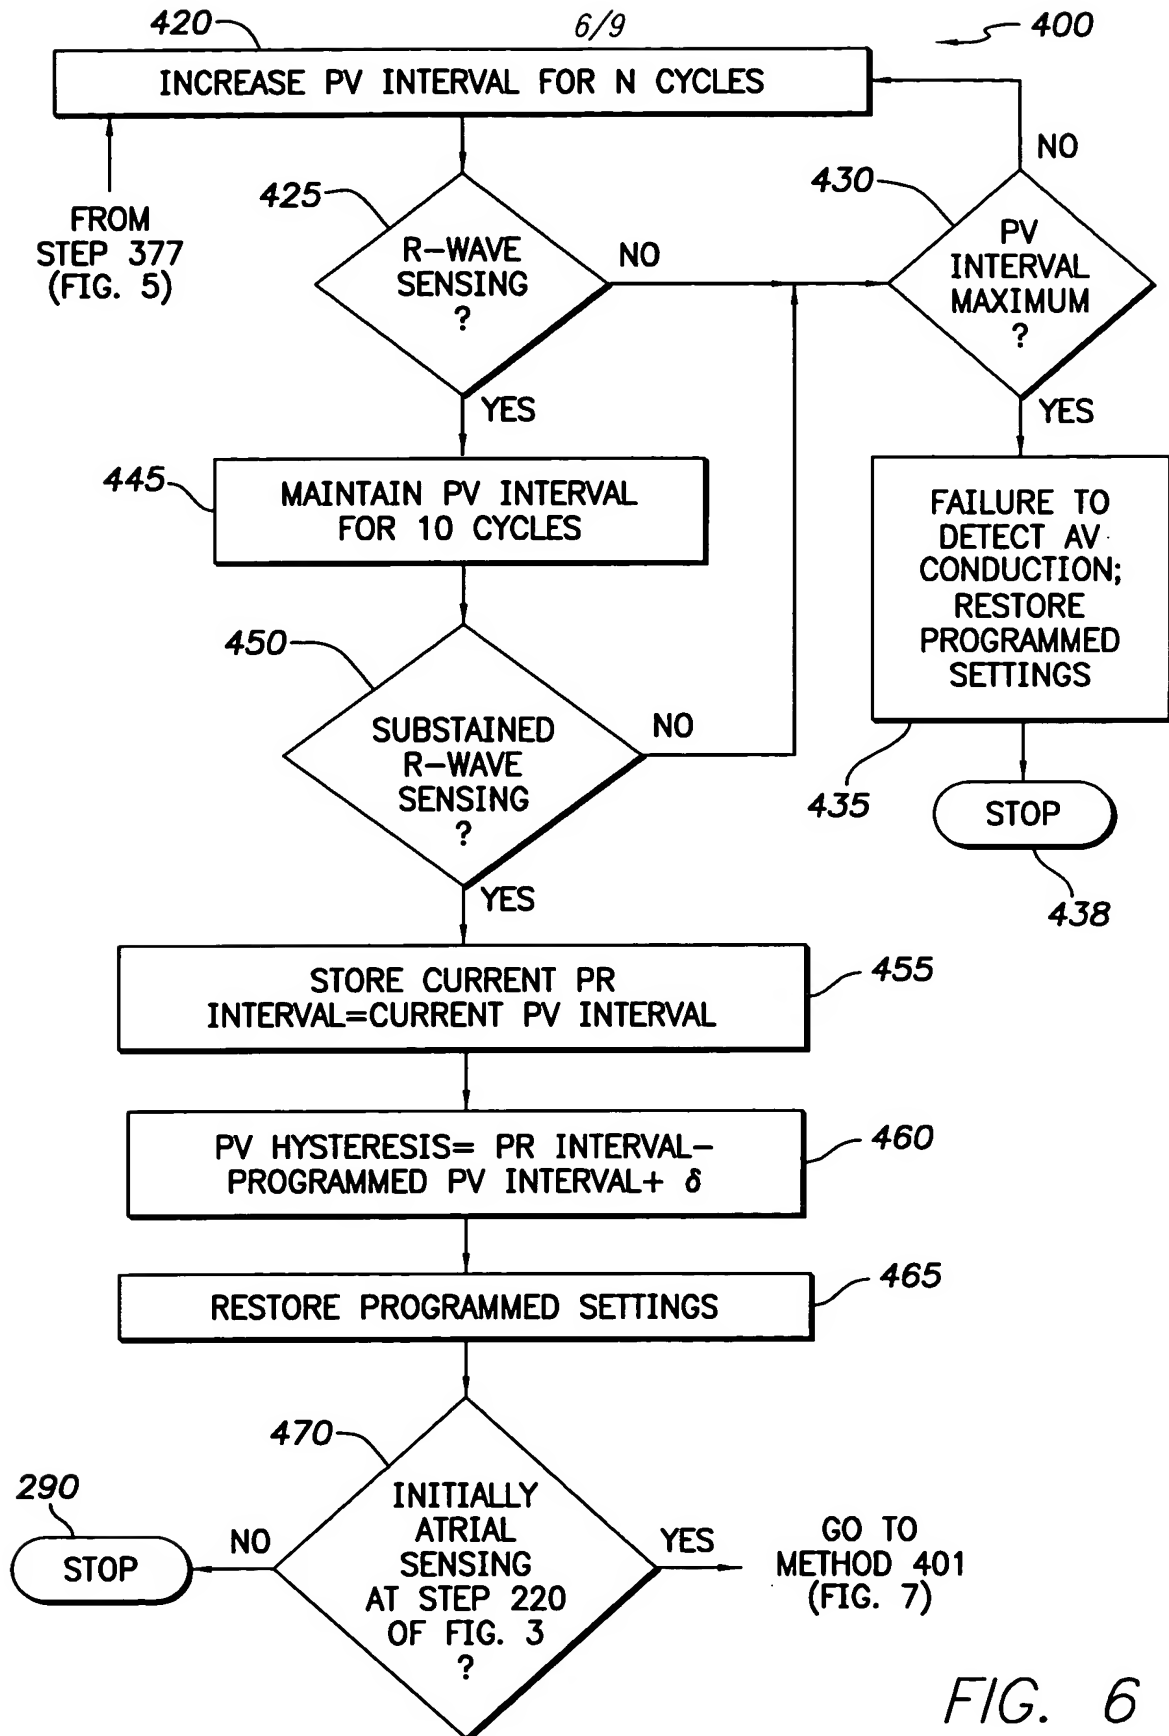
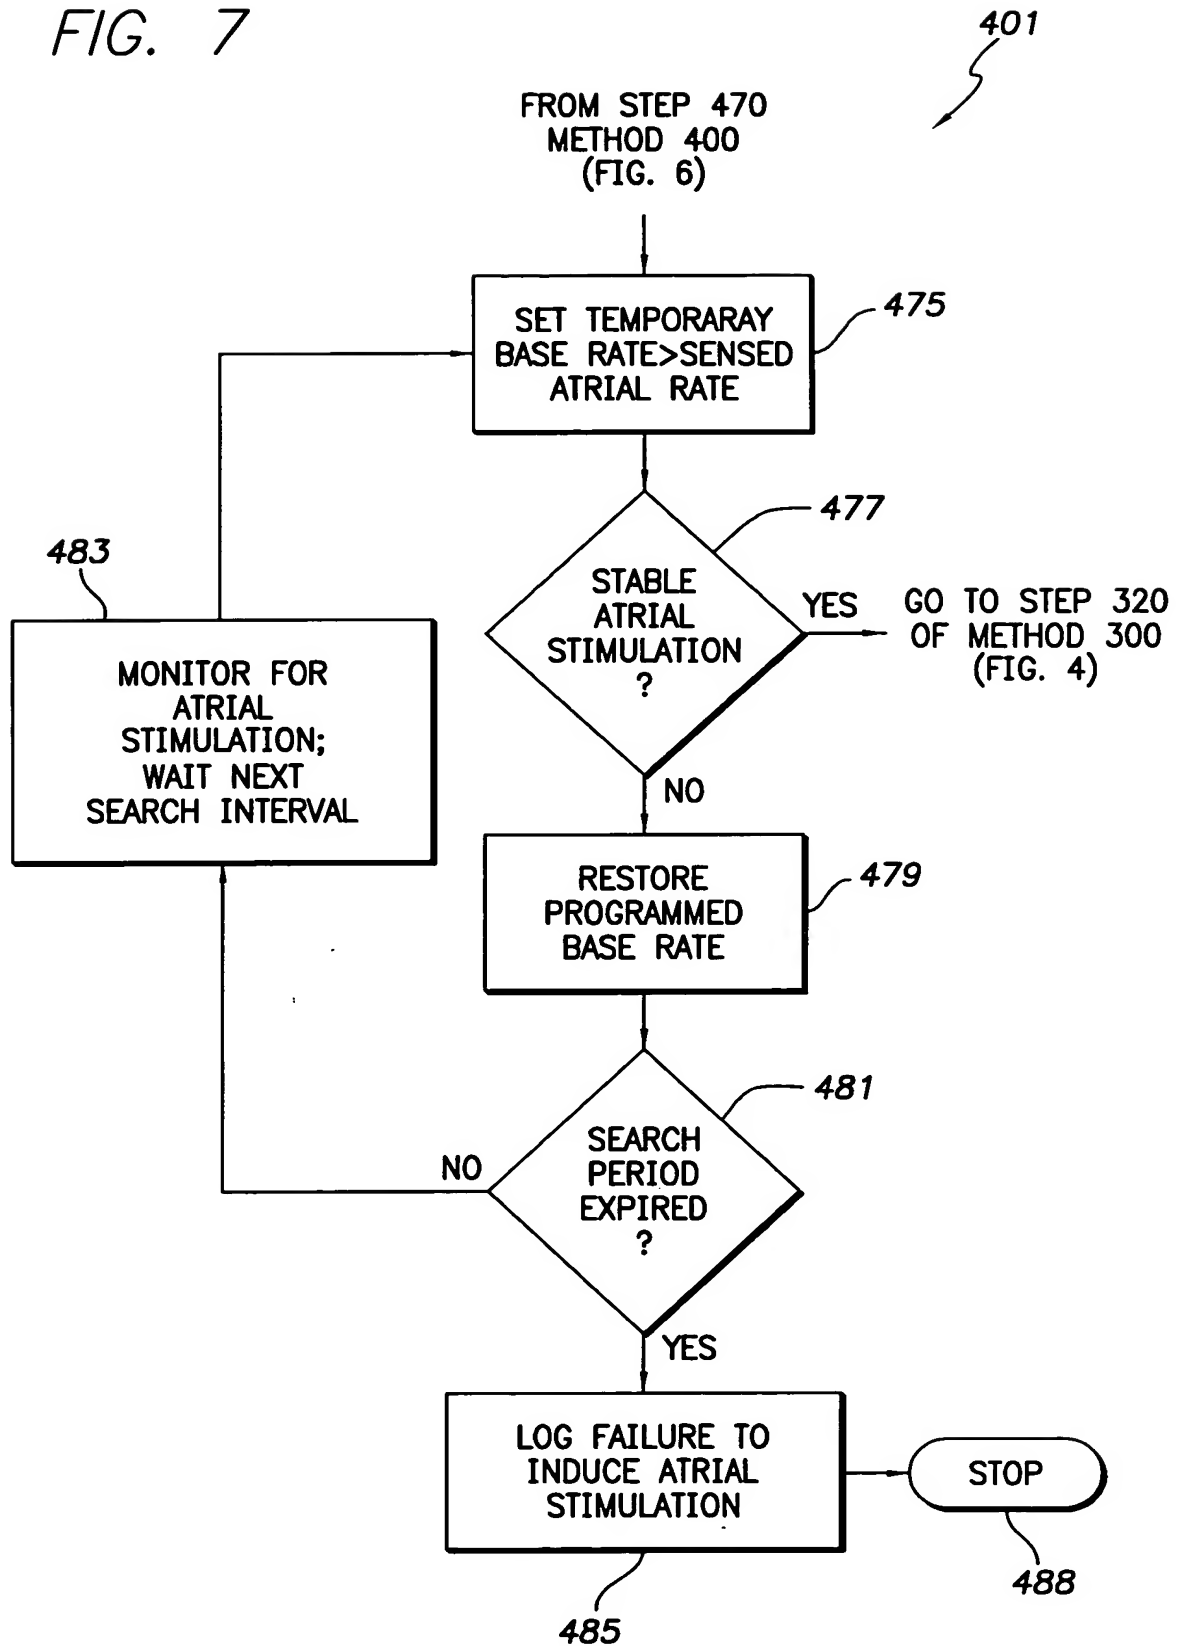


FIG. 6

FIG. 7



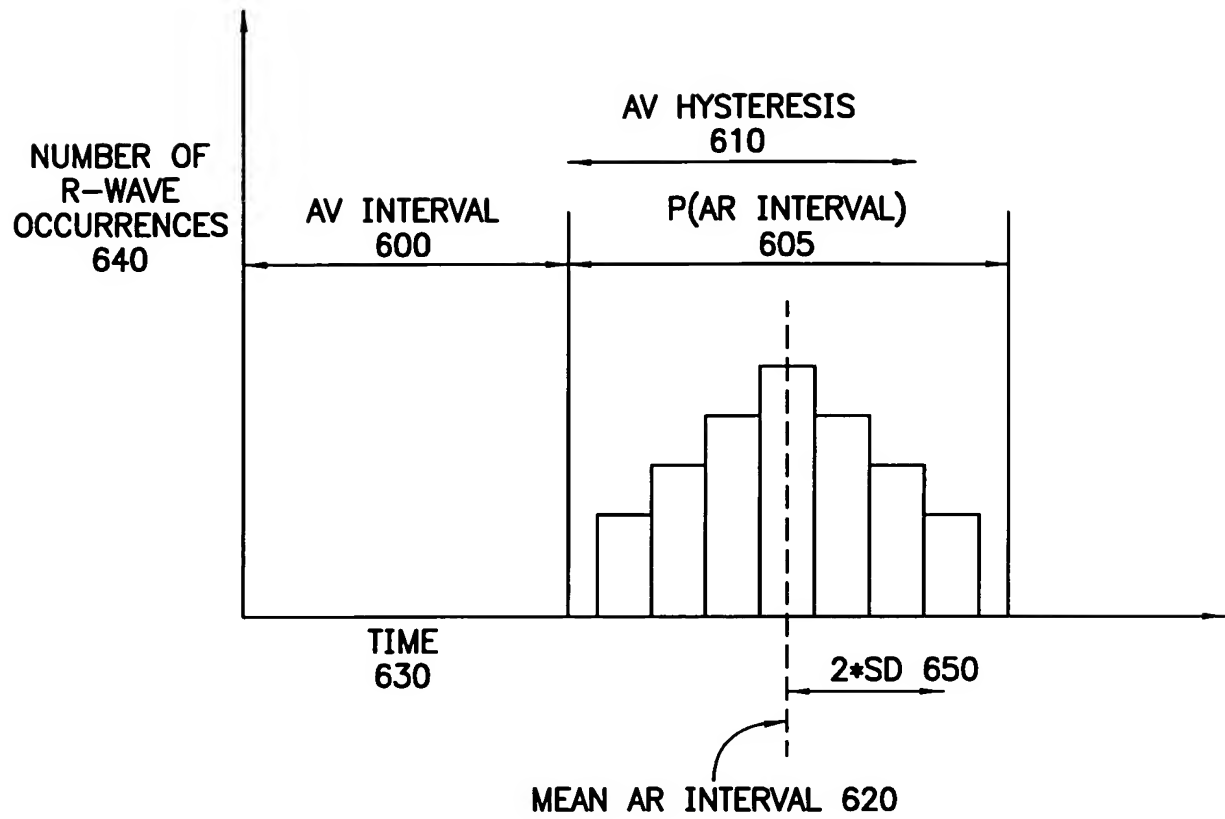


FIG. 8

9/9

FROM STEP 350,
(FIG. 4)

355 STORE CURRENT AR
INTERVAL=CURRENT
AV INTERVAL

710 SET
AV HYSTERESIS=AR INTERVAL-
PROGRAMMED AV INTERVAL+ δ
FOR 16 CARDIAC CYCLES WHILE MEASURING
THE MEAN AR INTERVAL
AND
THE MEAN AR INTERVAL'S STANDARD
DEVIATION (SD)

720 STORE THE MEAN AR INTERVAL
AND THE STANDARD DEVIATION (SD)

725 AV HYSTERESIS=MEAN AR INTERVAL
+ 2*SD -AV INTERVAL

365 RESTORE PROGRAMMED SETTINGS



FIG. 9